

MammoView 1.5

DICOM Conformance Statement 1.0

© medigration GmbH
All rights reserved

Table of Contents

1	Introduction	4
1.1	Purpose	4
1.2	Scope	4
1.3	Definitions, Acronyms and Abbreviations	5
1.3.1	Definitions	5
1.3.2	Acronyms and Abbreviations	5
1.4	References	5
2	Implementation Model.....	6
2.1	Application Data Flow Diagram	6
2.2	Functional Definition of Application Entities	7
2.3	Sequencing of Real World Activities	7
3	MammoView Application Entity Specification	8
3.1	MammoView Specification.....	8
3.1.1	Association Establishment Policies.....	9
3.1.1.1	General	9
3.1.1.2	Number of Associations	10
3.1.1.3	Implementation Identifying Information.....	10
3.1.2	Association Initiation Policy	10
3.1.2.1	User Initiated Image Send	10
3.1.2.1.1	Associated Real-World Activity (User Send)	10
3.1.2.1.2	Proposed Presentation Contexts	10
3.1.2.1.3	SOP Specific Conformance	11
3.1.2.1.4	Association Termination.....	12
3.1.2.2	Print Images.....	12
3.1.2.2.1	Associated Real-World Activity (Send PrintJob).....	12
3.1.2.2.2	Proposed Presentation Contexts	12
3.1.2.2.3	SOP Specific Conformance	13
3.1.2.2.3.1	Conformance for Basic Film Session SOP Class	13
3.1.2.2.3.2	Conformance for Basic Film Box SOP Class.....	13
3.1.2.2.3.3	Conformance for the Basic Grayscale Image Box SOP Class	14
3.1.2.2.3.4	Conformance for Presentation LUT SOP Class	15
3.1.2.2.4	Association Termination.....	15
3.1.3	Association Acceptance Policy	16
3.1.3.1	Respond to Communication Verification Requests	16
3.1.3.1.1	Associated Real-World Activity.....	16
3.1.3.1.2	Acceptable Presentation Contexts	16
3.1.3.1.3	SOP Specific Conformance	16
3.1.3.1.4	Presentation Context Acceptance Criteria.....	16
3.1.3.1.5	Transfer Syntax Selection Policies	17
3.1.3.2	Receive DCOs for Storage	17
3.1.3.2.1	Associated Real-World Activity.....	17

3.1.3.2.2	Acceptable Presentation Contexts	17
3.1.3.2.3	SOP Specific Conformance	17
3.1.3.2.4	Presentation Context Acceptance Criteria	18
3.1.3.2.5	Transfer Syntax Selection Policies	18
4	Communication Profiles	19
4.1	Supported Communication Stacks	19
4.1.1	TCP/IP Stack	19
4.1.1.1	Physical Network Media Support	19
5	Configuration	19
6	Support of Extended Character Sets	20
	List of Tables	21
	Historie	21

1 Introduction

1.1 Purpose

A DICOM Conformance Statement is intended to describe which components, optional components or extensions of the DICOM standard are supported by a particular implementation. The Conformance Statement of one implementation can be compared with the Conformance Statement from another implementation to determine which capabilities are commonly supported.

DICOM does not, by itself, guarantee interoperability. Furthermore, the identification of common capabilities by comparing DICOM Conformance Statements is also not sufficient to guarantee connectivity between two devices.

A DICOM Conformance Statement cannot replace validation and cross-vendor testing with other devices. Validation and cross-vendor testing are still required to ensure that both devices are performing as intended.

The reader should be aware of a number of important issues:

- Even when comparing this Conformance Statement with the Conformance Statement of another device indicates that connectivity is possible, the system integrator is responsible for carrying out test procedures to ensure that the required connectivity is actually met.
- Neither the DICOM Standard nor this Conformance Statement can ensure interoperability when integrating devices from different vendors. It is the system integrator's responsibility to ensure that the application requirements of all devices within the complete system are met.
- The DICOM standard undergoes continual review and improvement in order to meet changing requirements. Corrections, extensions and additional services are added from time to time. Medigration reserves the right to make changes to the product described in this conformance statement in order to cover changes in the DICOM standard. Readers should be aware that connected devices should also follow changes in the DICOM standard in order to retain connectivity.

The intended audience for this Conformance Statement is hospital technical staff, system integrators and software engineers. The reader is assumed to have good understanding of the DICOM standard.

1.2 Scope

This conformance statement describes the DICOM capabilities of the medigration MammoView. The MammoView is a diagnostic workstation for medical mammographic images. It is specifically designed to be integrated into a DICOM network environment containing Modalities and Archives from different vendors. It supports those DICOM services needed to receive images and other DCOs for display, to send images to another DICOM device and to print images to a hardcopy device (e.g. film camera).

1.3 Definitions, Acronyms and Abbreviations

1.3.1 Definitions

System Integrator	A person or organization responsible for integrating devices into a new or existing system. The System Integrator takes responsibility for ensuring that the system works as a whole.
-------------------	---

Other definitions can be found within the different parts of the DICOM standard [1]
DICOM, PS3.(1-18)-2009, National Electrical Manufacturers Association, 1300 N.
17th Street Rosslyn, Virginia 22209, USA..

1.3.2 Acronyms and Abbreviations

AE	Application Entity
DCO	DICOM Composite Object. A DICOM object such as an image, overlay, lookup-table, waveform, presentation state or radiotherapy plan which can be stored using the Storage Service Class.

1.4 References

[Ref. 1] [1] DICOM, PS3.(1-18)-2009, National Electrical Manufacturers Association,
1300 N. 17th Street Rosslyn, Virginia 22209, USA.

2 Implementation Model

The MammoView is a device for the storage and display of DICOM Composite Objects (DCOs). The objects which can be stored include a wide variety of DICOM images (e.g. CT, MR, US, etc.) and other objects (e.g. presentation states, radiotherapy objects, etc.). The MammoView software receives DCOs over a network interface, stores them on local magnetic disks and displays them on a monitor for diagnostic purpose. It is also capable of printing the images to a softcopy display. It maintains a database of summary information about stored objects and allows this database to be queried.

2.1 Application Data Flow Diagram

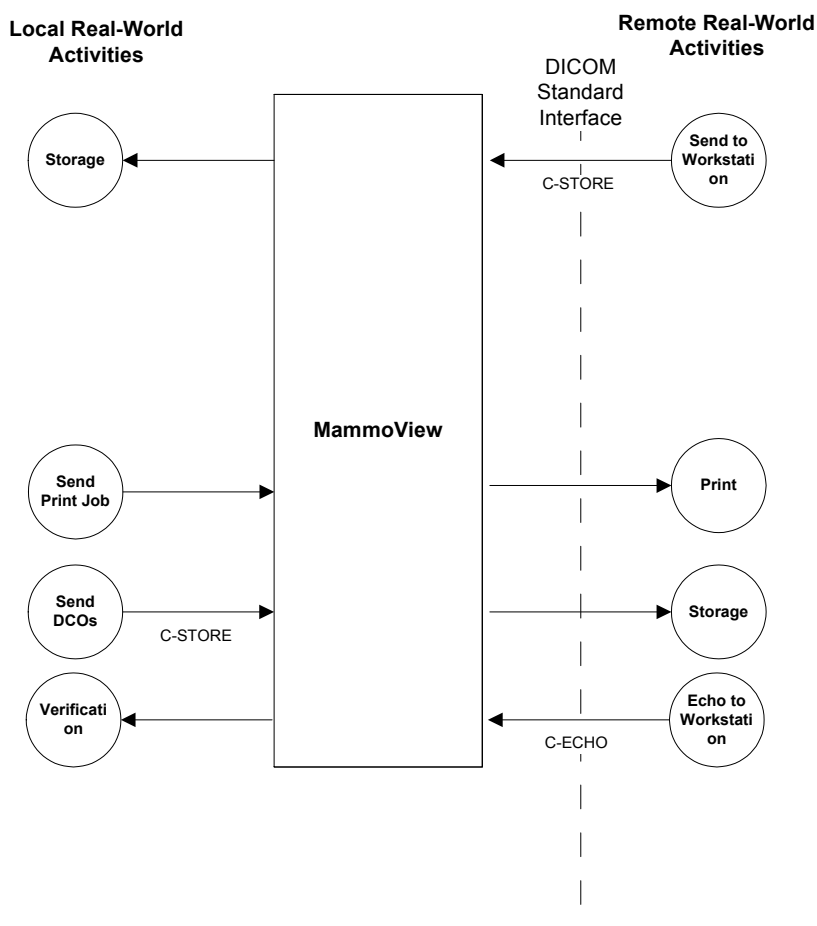


Figure 1: MammoView Implementation Model

Figure 1 illustrates the relationships between the MammoView Application Entity (AE) and its associated Real-World Activities. The **Remote Real-World Activities** are shown on the right and the **Local Real-World Activities** are shown on the left.

Send to Workstation is an activity performed by a remote device to send DCOs to the MammoView to be stored by the **Storage** local activity.

Print jobs can be send by the **Send Print Job** local activity to be printed by the **Print** activity on the remote device.

DCOs can be send by the **Send** local activity upon operator request. They are stored by the **Storage** activity on the remote device.

Echo to Workstation is an activity performed by a remote device to verify communication with ImageVision. The local activity performed by ImageVision is **Verification**.

2.2 Functional Definition of Application Entities

The MammoView software acts as a single Application Entity (AE) providing a general display service for medical images and other related objects. The AE is able to receive images for storage and to send images and other objects to remote devices. It also can send print jobs to other devices to generate hardcopies of the images.

The MammoView acts as an SCU of the following DICOM Service Classes:

- Storage
- Basic Grayscale Print Management

The MammoView acts as an SCP of the following DICOM Service Classes:

- Storage
- Verification

2.3 Sequencing of Real World Activities

No sequencing of Real-World activities is relevant.

3 MammoView Application Entity Specification

3.1 MammoView Specification

The MammoView provides standard conformance to the Storage Service class by supporting the SOP Classes and roles listed in Table 1: Supported DICOM Storage SOP Classes and Roles.

SOP Class Name	UID	Role
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	SCU/SCP
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	SCU/SCP
Hardcopy Color Image Storage	1.2.840.10008.5.1.1.30	SCU/SCP
Hardcopy Grayscale Image Storage	1.2.840.10008.5.1.1.29	SCU/SCP
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	SCU/SCP
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	SCU/SCP
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	SCU/SCP
Raw Data Storage	1.2.840.10008.5.1.4.1.1.4.2	SCU/SCP
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	SCU/SCP
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	SCU/SCP
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	SCU/SCP
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	SCU/SCP
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	SCU/SCP
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	SCU/SCP
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	SCU/SCP
RT Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6	SCU/SCP
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	SCU/SCP
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	SCU/SCP
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	SCU/SCP
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	SCU/SCP
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	SCU/SCP
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	SCU/SCP
Stand-alone Curve Storage	1.2.840.10008.5.1.4.1.1.9	SCU/SCP
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	SCU/SCP
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	SCU/SCP
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	SCU/SCP
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	SCU/SCP
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	SCU/SCP

Storage		
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	SCU/SCP
Stand-alone Modality LUT Storage	1.2.840.10008.5.1.4.1.1.10	SCU/SCP
Stand-alone Overlay Storage	1.2.840.10008.5.1.4.1.1.8	SCU/SCP
Stand-alone VOI LUT Storage	1.2.840.10008.5.1.4.1.1.11	SCU/SCP
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	SCU/SCP
Standalone PET Curve Storage	1.2.840.10008.5.1.4.1.1.129	SCU/SCP
Stored Print Storage	1.2.840.10008.5.1.1.27	SCU/SCP
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	SCU/SCP
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	SCU/SCP
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	SCU/SCP
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	SCU/SCP
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	SCU/SCP
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	SCU/SCP
Digital Mammography X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	SCU/SCP
Digital Mammography X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	SCU/SCP
Digital Intra-oral X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	SCU/SCP
Digital Intra-oral X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	SCU/SCP
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	SCU/SCP
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	SCU/SCP
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	SCU/SCP
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	SCU/SCP
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	SCU/SCP
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	SCU/SCP
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	SCU/SCP
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	SCU/SCP
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	SCU/SCP
Key Object Selection	1.2.840.10008.5.1.4.1.1.88.59	SCU/SCP

Table 1: Supported DICOM Storage SOP Classes and Roles

3.1.1 Association Establishment Policies

3.1.1.1 General

All relevant DICOM communication parameters (AE Titles, hostnames or IP addresses, port numbers, etc.) are configurable. See section 5 for more information on configurable

parameters. A maximum PDU size of 16KB will be offered when establishing associations. Any maximum PDU size will be accepted although PDU sizes larger than 64k will never be sent.

3.1.1.2 Number of Associations

The number of concurrent associations which can be accepted is configurable. See section 5 for more information on configurable parameters.

No fixed limit exists on the number of associations which can be initiated other than the resource limits imposed by the underlying operating system. In the following cases associations will be initiated by the MammoView:

- for sending DCOs by explicit operator action
- to send print jobs to a printer

3.1.1.3 Implementation Identifying Information

Implementation Class UID:	1.2.276.0.7230010.3.0.3.5.4
Implementation Version Name:	OFFIS_DCMTK_354

3.1.2 Association Initiation Policy

The MammoView will initiate associations in the following situations:

- When instructed by an operator (via the user interface) to send DCOs to a remote device.
- When instructed by an operator (via the user interface) to print images.

3.1.2.1 User Initiated Image Send

3.1.2.1.1 Associated Real-World Activity (User Send)

An operator can - via a graphical user interface - initiate sending images to a remote application entity. The associated local real-world activity is **User Send** and the remote real world activity is **Storage**. The operator can select any appropriate grouping of images (e.g. all patient images, all images of specific studies, selected series, individual images, etc.). All selected images will be sent over a single association.

3.1.2.1.2 Proposed Presentation Contexts

One or more presentation contexts will be proposed for *user initiated image send* as outlined in Table 1: Supported DICOM Storage SOP Classes and Roles. However, only those Storage SOP Classes of images to actually be sent will be proposed (e.g. if only CT images are to be

sent then only the CT Image Storage SOP Class will be proposed as an abstract syntax). Each abstract syntax will be proposed within at least 2 presentation contexts using different transfer syntax subsets. The presentation context proposal policy attempts to propose abstract syntax / transfer syntax combinations such that the original transfer syntax of received images can be maintained when sending images. This behavior is intended to eliminate transfer syntax conversion wherever possible.

The presentation context proposal policy can be modified by configuration options so that only the default transfer syntax (Implicit VR Little Endian) is proposed during association negotiation with specific application entities.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Any of the Storage SOP Class names listed in Table 1: Supported DICOM Storage SOP Classes and Roles.	Any of the Storage SOP Class UIDs listed in Table 1: Supported DICOM Storage SOP Classes and Roles.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Table 2: Proposed presentation contexts for operator initiated image send

3.1.2.1.3 SOP Specific Conformance

The behavior when receiving C-STORE response status codes is shown in Table 3: Behavior when receiving C-STORE response status codes (operator initiated)

. The operator will be informed by posting a message to the operator's user interface message area.

Status Code	Meaning	Behavior when receiving status code
	Any other status code not included in this table	The send activity will be terminated (the remaining images will not be sent). An error message will be posted to the operator and an error message recorded in a log file.
A7xx	Refused – Out of Resources	
A9xx	Error – Data Set does not match SOP Class	The remaining images will be sent if possible. An error message will be posted to the operator and an error message recorded in a log file.
Cxxx	Error – Cannot Understand	

B000	Warning – Coercion of Data Elements	The operator will be informed after all images have been sent.
B007	Warning – Data Set does not match SOP Class	
B006	Warning – Elements Discarded	
0000	Success	

Table 3: Behavior when receiving C-STORE response status codes (operator initiated)

Extended negotiation is not supported for the *User Send* Real-World Activity. All optional attributes included in Storage SOP Instances will be sent as originally received. Storage SOP Instances are stored without modification when received and are not modified when sent. No additional attributes are added.

3.1.2.1.4 Association Termination

The association will be released upon receipt of the C-STORE-RSP message for the last sent image or upon receipt of refused or unknown status code.

If the peer AE aborts the association prematurely, all unsent SOP Instances are considered failed.

3.1.2.2 Print Images

3.1.2.2.1 Associated Real-World Activity (*Send PrintJob*)

The user can select a set of images to be printed to a remote dicom printer. The resulting hardcopy can be printed on transmissive (film) or reflective (paper) media. The associated local real-world activity is **Send PrintJob** and the remote real world activity is **Print**.

3.1.2.2.2 Proposed Presentation Contexts

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None

		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Presentation LUT	1.2.840.10008.5.1.1.23	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

Table 4: Proposed presentation contexts for an operator initiated print request

3.1.2.2.3 *SOP Specific Conformance*

MammoView supports the SOP Classes listed in Table 5 as defined by the Basic Grayscale Print Management Meta SOP Class.

SOP Class Name	SOP Class UID
Basic Film Session	1.2.840.10008.5.1.1.1
Basic Film Box	1.2.840.10008.5.1.1.2
Basic Grayscale Image Box	1.2.840.10008.5.1.1.4
Printer	1.2.840.10008.5.1.1.16

Table 5: Supported SOP Classes for the Basic Grayscale Print Management Meta SOP Class

Extended negotiation is not supported for the *Send PrintJob* Real-World Activity.

3.1.2.2.3.1 **Conformance for Basic Film Session SOP Class**

MammoView includes the attributes from Table 6 in the N-CREATE request for the Basic Film Session SOP Class.

Attribute	Tag	Comment
Number of Copies	(2000,0010)	1
Print Priority	(2000,0020)	MED
Medium Type	(2000,0030)	<configurable>
Film Destination	(2000,0040)	<configurable>
Film Session Label	(2000,0050)	<configurable>

Table 6: Attributes for the Basic Film Session SOP Class

The N-SET and N-ACTION commands for the Basic Film Session SOP Class are unused. The N-DELETE command is used to delete the Film Session after all Film Boxes have been deleted.

3.1.2.2.3.2 **Conformance for Basic Film Box SOP Class**

MammoView includes the attributes from Table 7 in the N-CREATE request for the Basic Film Box SOP Class.

Attribute	Tag	Comment
Image Display Format	(2010,0010)	STANDARD\1,1
Referenced Film Session Sequence	(2010,0500)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
Film Orientation	(2010,0040)	PORTRAIT
Film Size ID	(2010,0050)	
Magnification Type	(2010,0060)	<configurable>
Max Density	(2010,0130)	<configurable>
Smoothing Type	(2010,0080)	<configurable>
Border Density	(2010,0100)	<configurable>
Empty Image Density	(2010,0110)	<configurable>
Min Density	(2010,0120)	<configurable>
Trim	(2010,0140)	<configurable>
Referenced Presentation LUT Sequence	(2050,0500)	Will be sent if the Presentation LUT SOP Class was negotiated and a Presentation LUT SOP instance has successfully been created.
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	

Table 7: Attributes for the Basic Film Box SOP Class

The N-SET and N-ACTION commands for the Basic Film Box SOP Class are unused. The N-DELETE command is used to delete the Film Box with all Image Boxes managed by the Film Box.

3.1.2.2.3.3 Conformance for the Basic Grayscale Image Box SOP Class

MammoView includes the attributes from Table 8 in the N-CREATE request for the Basic Grayscale Image Box SOP Class.

Attribute	Tag	Comment
ImagePosition	(2020,0010)	1
Basic Grayscale Image Sequence	(2020,0110)	Only a single item is present.
> Samples Per Pixel	(0028,0002)	1
> Photometric Interpretation	(0028,0004)	
> Rows	(0028,0010)	Depends on the resolution of the display device. Configurable.
> Columns	(0028,0011)	Depends on the resolution of the display device. Configurable.
> Pixel Aspect Ratio	(0028,0034)	
> Bits Allocated	(0028,0100)	8
> Bits Stored	(0028,0101)	8
> High Bit	(0028,0102)	7
> Pixel Representation	(0028,0103)	0
> Pixel Data	(7FE0,0010)	

Table 8: Attributes for the Basic Grayscale Image Box SOP Class

The N-SET and N-ACTION commands for the Basic Grayscale Image Session SOP Class are unused.

3.1.2.2.3.4 Conformance for Presentation LUT SOP Class

MammoView includes the attributes from Table 9 in the N-CREATE request for the Presentation LUT SOP Class.

Attribute	Tag	Comment
Presentation LUT Shape	(2050,0010)	IDENTITY

Table 9: Attributes for the Presentation LUT SOP Class

The N-SET and N-ACTION commands for the Presentation LUT SOP Class are unused. The N-DELETE command is used to delete the Presentation LUT for the current Basic Film Box or Film Session.

3.1.2.2.4 Association Termination

The association will be released upon receipt of the N-DELETE-RSP of the Basic Film Session.

3.1.3 Association Acceptance Policy

The MammoView application will accept associations for the following situations:

- To respond to communication verification requests from remote devices.
- To receive DCOs for storage from remote devices.

Associations can be accepted at any time the MammoView application entity is active. The MammoView application entity may not be active if stopped or restarted by an operator.

Associations will be terminated (A-ABORT) if they are idle for more than 20 minutes.

3.1.3.1 Respond to Communication Verification Requests

3.1.3.1.1 Associated Real-World Activity

An association will be accepted from a remote Application Entity in order to respond to communication verification requests. The local real-world activity is **Verification** and the remote real world activity is **Echo to Workstation**.

3.1.3.1.2 Acceptable Presentation Contexts

Any of the presentation contexts shown in Table 10: Acceptable presentation context for Verification can be accepted.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Table 10: Acceptable presentation context for Verification

3.1.3.1.3 SOP Specific Conformance

Standard conformance is provided for the Verification SOP Class.

3.1.3.1.4 Presentation Context Acceptance Criteria

A presentation context for the Verification SOP Class will always be accepted provided the transfer syntax selection policy is met. Presentation contexts for other supported activities may also be accepted on the same association.

3.1.3.1.5 *Transfer Syntax Selection Policies*

Only the default DICOM Transfer Syntax (Implicit VR Little Endian) will be accepted.

3.1.3.2 Receive DCOs for Storage

An association will be accepted from a remote Application Entity in order to receive images for storage. The local real-world activity is **Storage** and the remote real world activity is **Send to Workstation**.

Received images are stored on local disk, summary information extracted from the image and inserted in a central database. The extraction of summary information is tolerant of encoding errors wherever possible. Invalid attribute values will be retained in the image files but may be ignored or truncated when inserted into the central database.

3.1.3.2.1 *Associated Real-World Activity*

An association will be accepted from a remote Application Entity in order to receive images for storage. The local real-world activity is **Storage** and the remote real world activity is **Send to Workstation**.

Received images are stored on local disk, summary information extracted from the image and inserted in a central database. The extraction of summary information is tolerant of encoding errors wherever possible. Invalid attribute values will be retained in the image files but may be ignored or truncated when inserted into the central database.

3.1.3.2.2 *Acceptable Presentation Contexts*

Any of the presentation contexts shown in Table 11: Acceptable presentation contexts for storage can be accepted.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Any of the Storage SOP Class names listed in Table 1: Supported DICOM Storage SOP Classes and Roles.	Any of the Storage SOP Class UIDs listed in Table 1: Supported DICOM Storage SOP Classes and Roles.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Table 11: Acceptable presentation contexts for storage

3.1.3.2.3 *SOP Specific Conformance*

Conformance to the SOP Classes of the Storage Service Class is at Level 2 (Full). Moreover, all received attributes (Type 1, Type 2, Type 3 and Private) are stored without modification. No attributes are discarded. Received images are written to local disk using the DICOM File Format as specified in PS 3.10. The identity of the transfer syntax used to receive the image is recorded in the File Format meta header along with the Source Application Entity Title. No specific policies are required concerning the attribute Lossy Image Compression (0028,2110).

No automatic coercion of attribute values will be performed.

If a success or warning status is returned in a C-STORE response the image has been stored to local disk and registered in the central database. If an image is received containing a SOP Instance UID which is already stored in the database then a success status is returned and the image is updated.

The meaning of status codes which can be returned in a C-STORE response are listed in Table 12: C-STORE response status codes. More detailed error information may be provided in the related fields Offending Element (0000, 0901) and Error Comment (0000,0902).

Status Code	Meaning	Detail
A700	Refused – Out of Resources	Insufficient disk space is available or insufficient permissions exist to store the image. The image cannot be stored. An error message is recorded in a log file.
A900	Error – Data Set does not match SOP Class	A serious incompatibility between the dataset and the supposed SOP Class was detected. The image cannot be stored. An error message is recorded in a log file.
C000	Error – Cannot Understand	A serious error occurred while parsing the image or an error occurred while updating the database. The image cannot be stored. An error message is recorded in a log file.
0000	Success	The image has been successfully stored or an image with the same SOP Instance UID already exists. A message is recorded in a log file.

Table 12: C-STORE response status codes

3.1.3.2.4 Presentation Context Acceptance Criteria

Presentation contexts for any of the supported Storage SOP Classes will always be accepted provided the transfer syntax selection policy is met. Presentation contexts for other supported activities may also be accepted on the same association.

3.1.3.2.5 Transfer Syntax Selection Policies

Preference is by default given to receiving images encoded using an explicit transfer syntax. However, configuration options can be used to limit acceptance to only the default DICOM

Transfer Syntax (Implicit VR Little Endian) when accepting associations from specific application entities (see section 5 for configuration options).

When multiple Transfer Syntaxes are presented, a selection is made using following priority:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

4 Communication Profiles

4.1 Supported Communication Stacks

TCP/IP Network Communication is supported as defined in PS 3.8.

4.1.1 TCP/IP Stack

The TCP/IP stack is inherited from the underlying operating system.

4.1.1.1 Physical Network Media Support

No dependency exists on the physical network medium over which TCP/IP executes. The supported physical network media are inherited from the underlying operating system.

5 Configuration

The following DICOM-related network parameters are configurable by the user via a graphical user interface and are stored in the central database:

- The title of the MammoView Application Entity. Associations will not be accepted if the Called AE Title is not equal to the configured AE Title.
- The Port Number to use when listening for associations (default 104).
- The AE Titles, IP Address and Port Number for all peer application entities. These parameters must be configured before associations can be initiated or accepted. Association attempts from unknown AE Title and IP Address pairs will not be accepted.

- Support by peer application entities for the Verification SOP Class. If supported, a connectivity test can be performed upon user request.
- The preferred transfer syntax for each peer application entity. The transfer syntax selection policies can be configured such that only the Implicit VR Little Endian Transfer Syntax will be accepted for individual application entities.

The following DICOM-related network parameters are configurable by a field service engineer for the *Storage*, *Query/Retrieve*, *Retrieval Send*, *Echo Provider*, *Get Storage Commitment* and *Get MPPS* local activities:

- The number of concurrent associations which can be accepted (default 20). This limit is bound only by the availability of underlying operating system resources.
- General association inactivity timeout (default 1800 seconds).
- Timeout waiting for a DIMSE request (default 1200 seconds).
- Timeout waiting for a DIMSE response (default 300 seconds).
- Maximum size of a received PDU (default 16KB).

The *User Send* and *User Echo* local activities use timeout and maximum PDU size parameters with defaults as defined above but are not configurable by a field service engineer.

6 Support of Extended Character Sets

The following extended character sets are supported:

ISO-IR 100 Latin Alphabet Supplementary Set No. 1 (ISO 8859-1)

Note: The DICOM default character set (ISO-IR 6) is a subset of ISO-IR 100.

List of Tables

Table 1: Supported DICOM Storage SOP Classes and Roles 9
 Table 2: Proposed presentation contexts for operator initiated image send..... 11
 Table 3: Behavior when receiving C-STORE response status codes (operator initiated) 12
 Table 4: Proposed presentation contexts for an operator initiated print request..... 13
 Table 5: Supported SOP Classes for the Basic Grayscale Print Management Meta SOP Class
 13
 Table 6: Attributes for the Basic Film Session SOP Class 13
 Table 7: Attributes for the Basic Film Box SOP Class 14
 Table 8: Attributes for the Basic Grayscale Image Box SOP Class..... 15
 Table 9: Attributes for the Presentation LUT SOP Class..... 15
 Table 10: Acceptable presentation context for Verification 16
 Table 11: Acceptable presentation contexts for storage..... 17
 Table 12: C-STORE response status codes..... 18

Historie

<i>Datum</i>	<i>Version</i>	<i>Autor</i>	<i>Beschreibung</i>
<i>MammoView 1.5</i>			
04.02.2011	1.0	Richter	Freigabe
22.02.2010	0.1	Richter	Dokument überarbeitet. DICOM film print ergänzt
<i>MammoView 1.0</i>			
28.10.2009	1.0	Richter	Released Version
23.10.2009	0.1	Richter	Start Document

Copyright © medigration GmbH 2010. All rights reserved. For internal use only.
Alle Rechte vorbehalten. Nur für internen Gebrauch.